



Operation of the Cobra Autosampler on the 8610V gas chromatograph

There are four identical standoffs

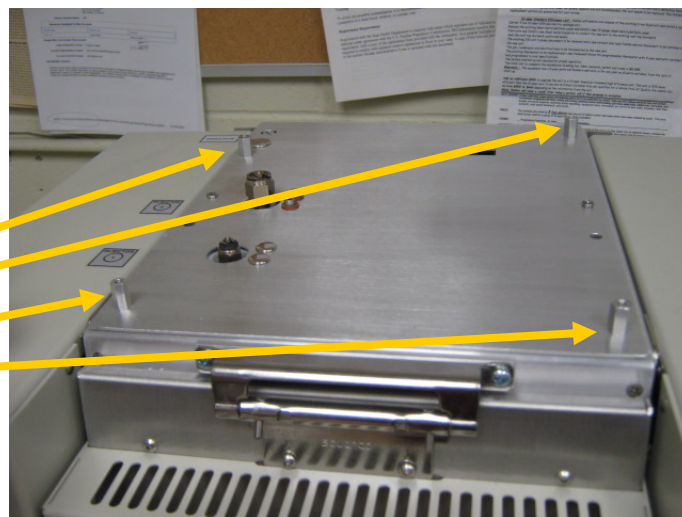

The autosampler plate has two locating pins.

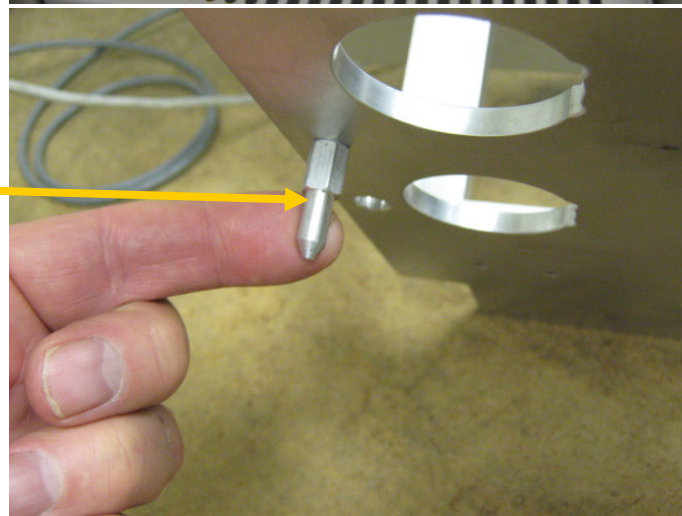

Lift the autosampler and plate onto the top of the 8610V GC.

