



Operation of the Cobra Autosampler on the 8610V gas chromatograph

Align the pins with the mating holes in the top of the GC.

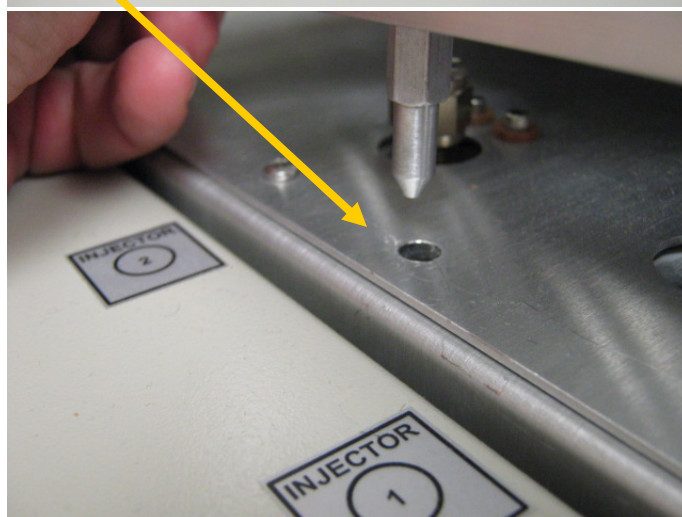

Secure the autosampler plate to the standoffs with the four brass thumbscrews.

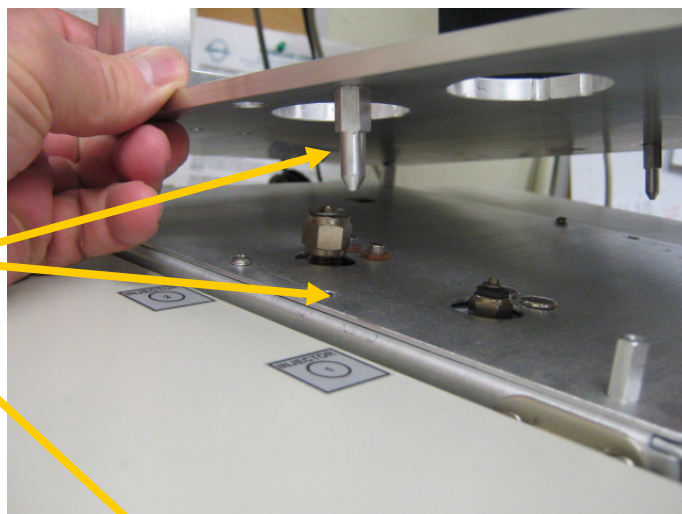