


Operation of the Cobra Autosampler on the 8610V gas chromatograph

Click Edit/Overall to display the Overall Controls screen.

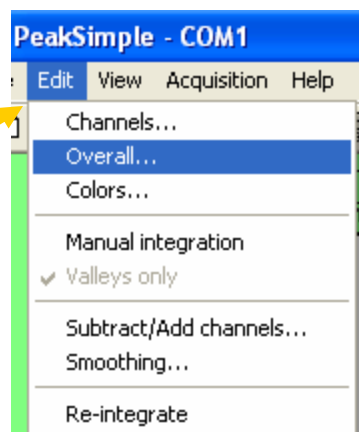

Remove the check mark from "Reset relays at end of run"

If you don't do this then Relay B will be turned off and the Cobra will not continue to run samples.

