


Operation of the Cobra Autosampler on the 8610V gas chromatograph

Verify that the lower needle support moves freely and that the syringe needle is still aligned in the lower support's guide hole.



Verify that the syringe needle finds the injector, sample, waste and rinse bottles. Be sure you have lined things up before you put the syringe in since any mis-alignment will result in a bent syringe needle.

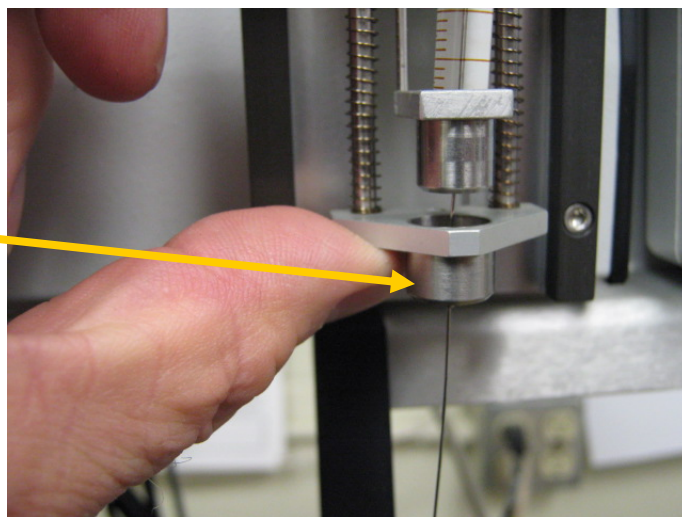