

Model 88 Methane/non-Methane GC

April 2019 (2020-9)

The SRI Model 88 GC is intended for measuring methane and non-methane hydrocarbons.




It can optionally be configured with a built-in hydrogen generator and air compressor like the one shown in the photo. This allows for completely gasless operation, a big convenience in some circumstances.

The valve oven, column and FID detector are mounted in this heated enclosure which can be set from ambient to 70°C.

The oven can NOT temperature program, it must be set to some isothermal temperature using the temperature controller mounted on the front panel.



The right side of the oven is removable for access to the parts inside.

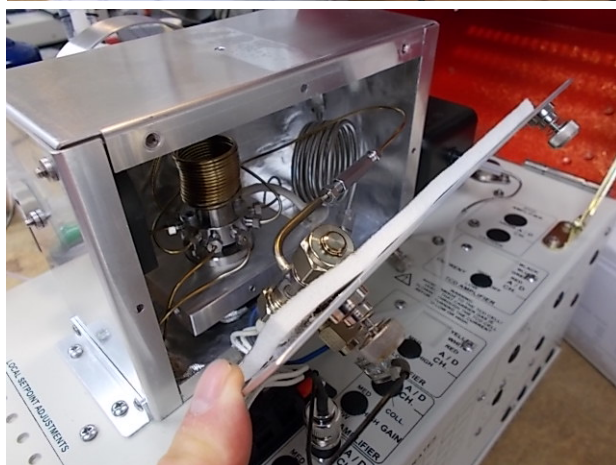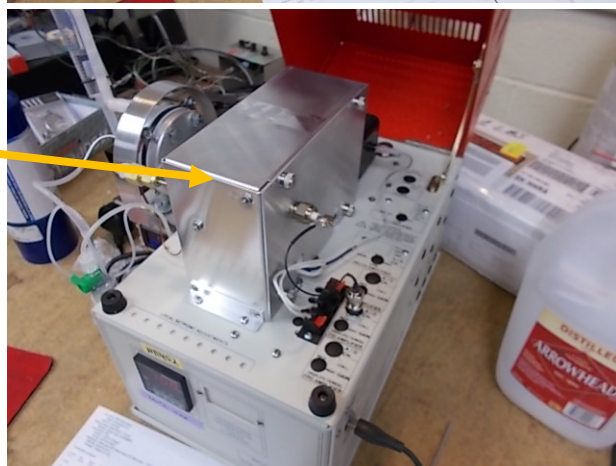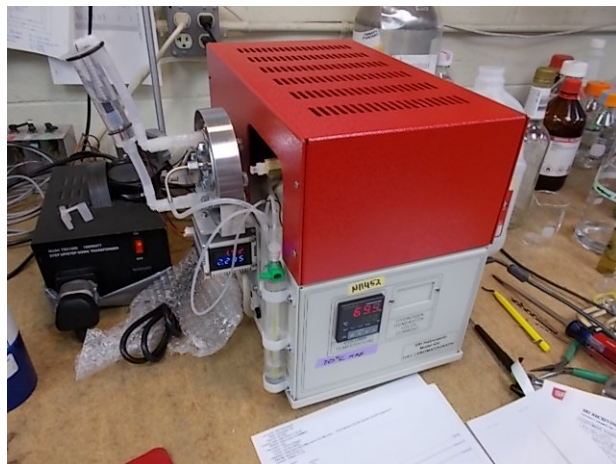

SRI Tech Support: 310-214-5092

www.srigc.com

Model 88 4-1-2019

Page 1

Model 88 Methane/non-Methane GC



April 2019

Inside the oven is the 10 port gas sampling valve with a 1ml loop, the 3 foot column, a circulation fan an FID detector and a heater block.

The circulation fan is what limits the oven temperature to 70C but it makes the temperature inside the oven more uniform.

The FID detector mounts to the removable side plate.

The collector electrode is on the right side, just above the connections for the ignitor and amplifier.

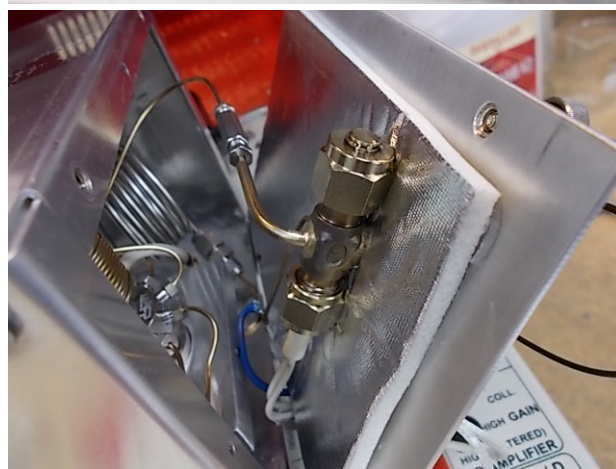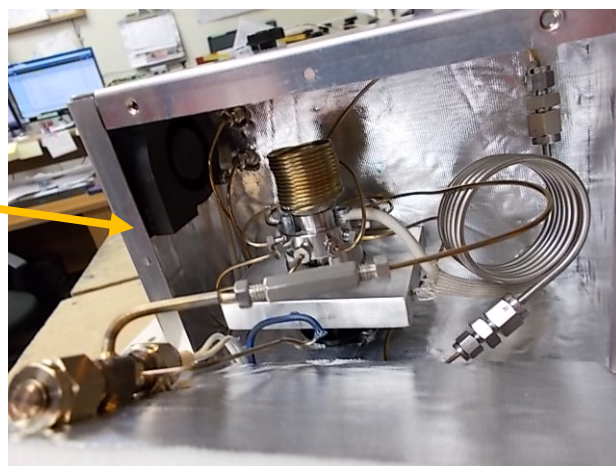

Model 88 4-1-2019

Page 2



Model 88 Methane/non-Methane GC

April 2019



The built-in hydrogen generator is mounted on the left and produces a steady 20ml/minute of H₂ carrier gas. The H₂ carrier is what also provides the H₂ for the FID detector.

A small air compressor provides combustion air for the FID detector.

The chromatogram looks like this.

The first peak is methane. The 2nd peak is ethane. The third large and wide peak is all the C₃ plus peaks after the valve was back-flushed at about 1.7 minutes.

You can also back-flush after methane for the C₂ plus instead of the C₃ plus.

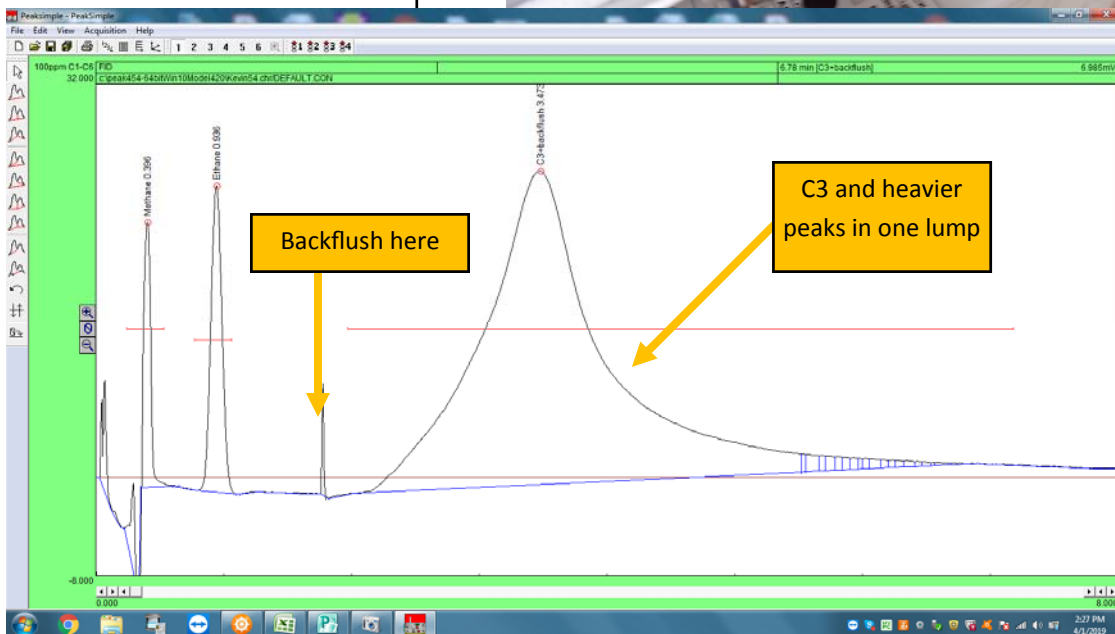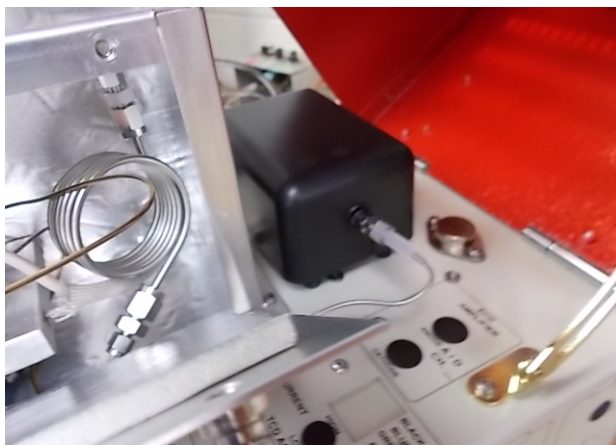

Model88 4-1-2019

Page 3

